

1/21

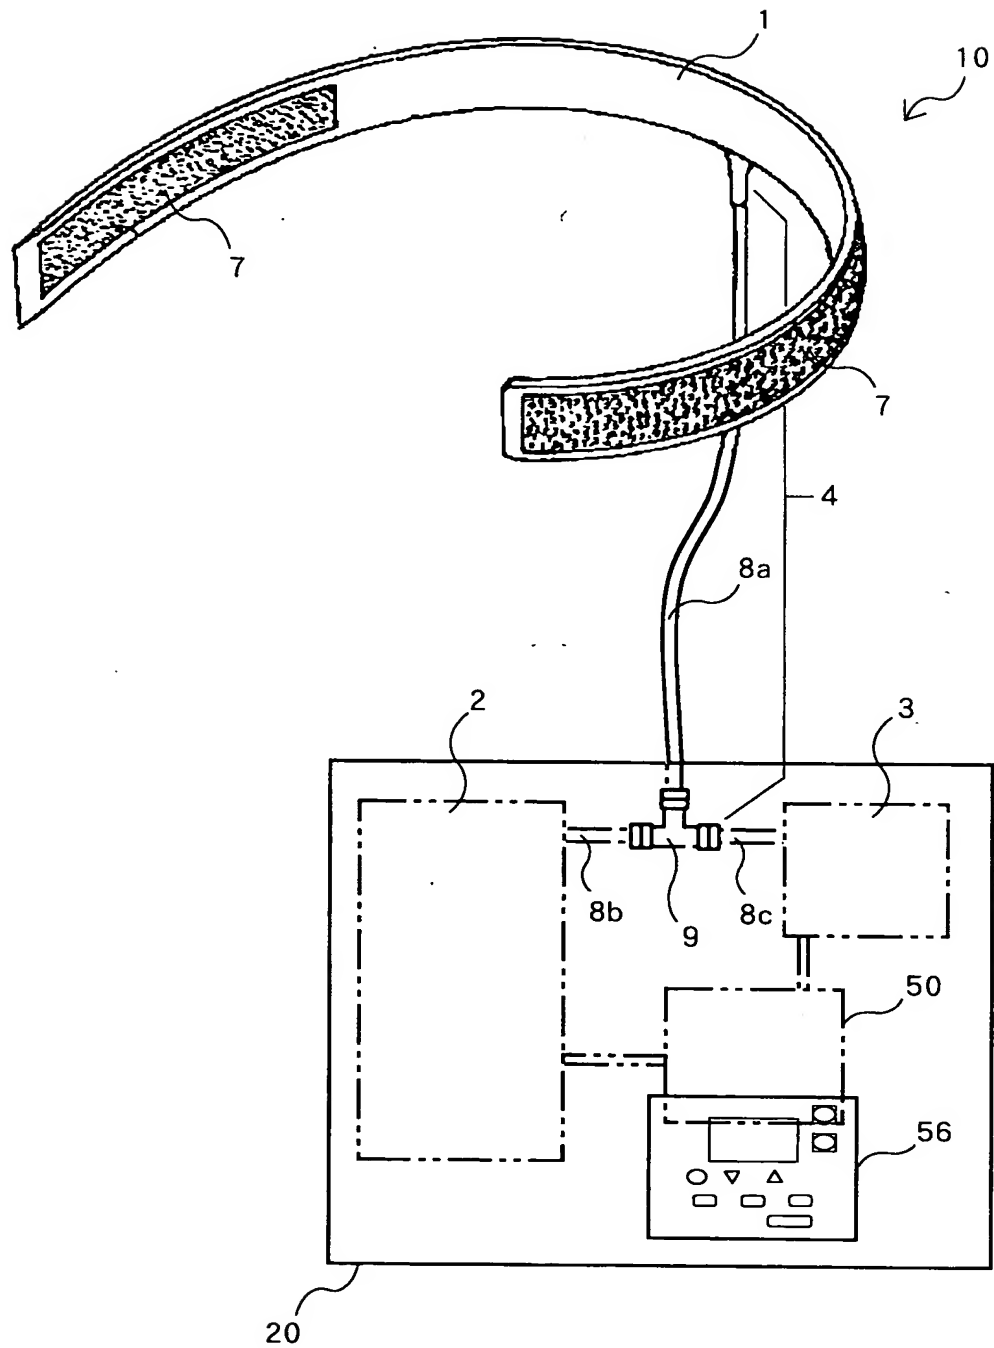


FIG. 1

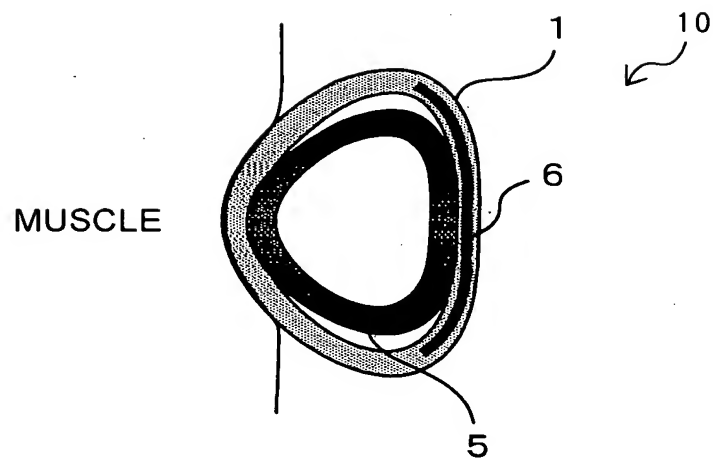


FIG. 2

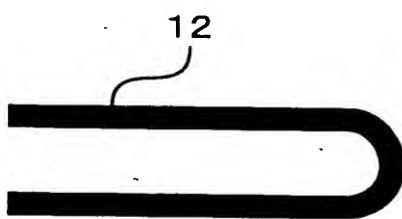


FIG. 3A

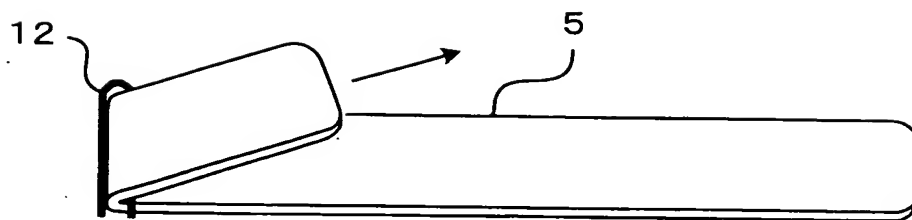


FIG. 3B

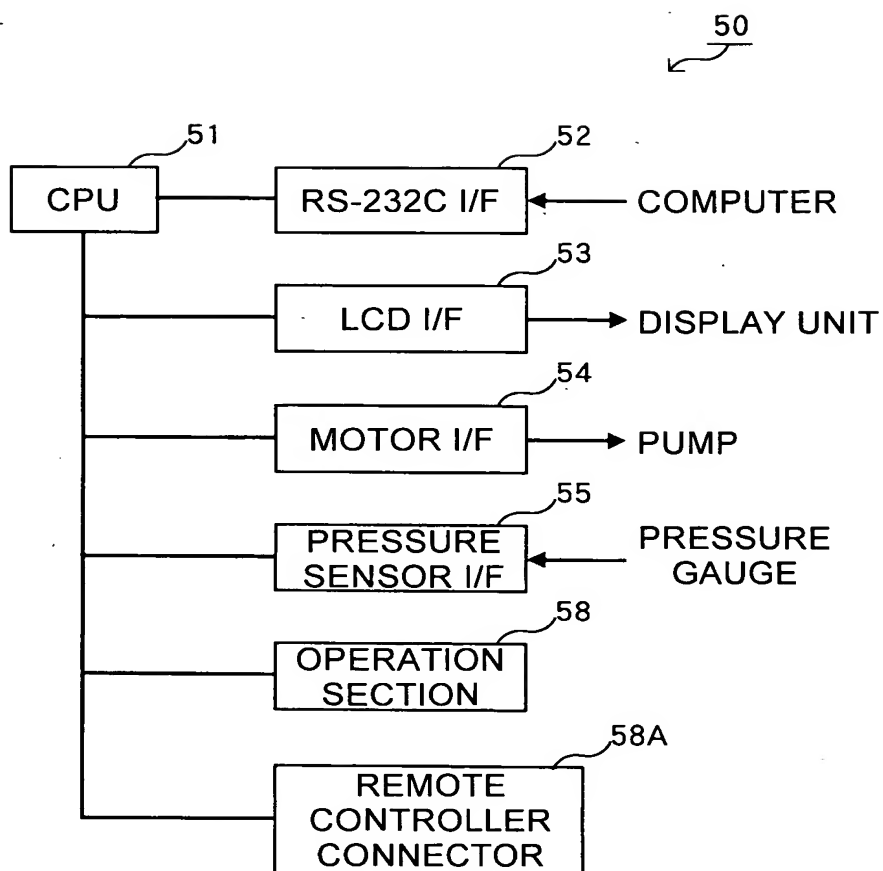


FIG. 4

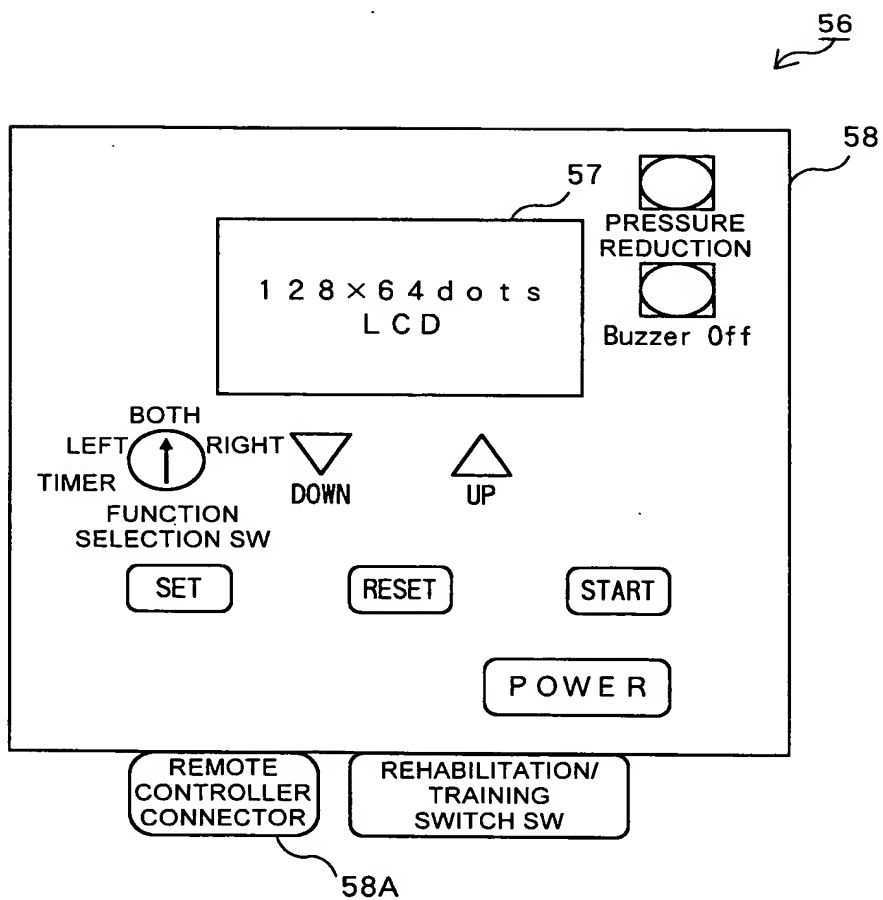


FIG. 5A

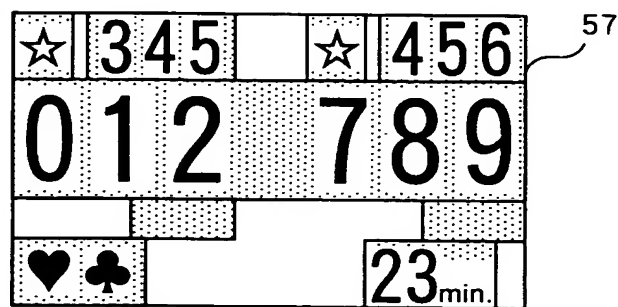


FIG. 5B

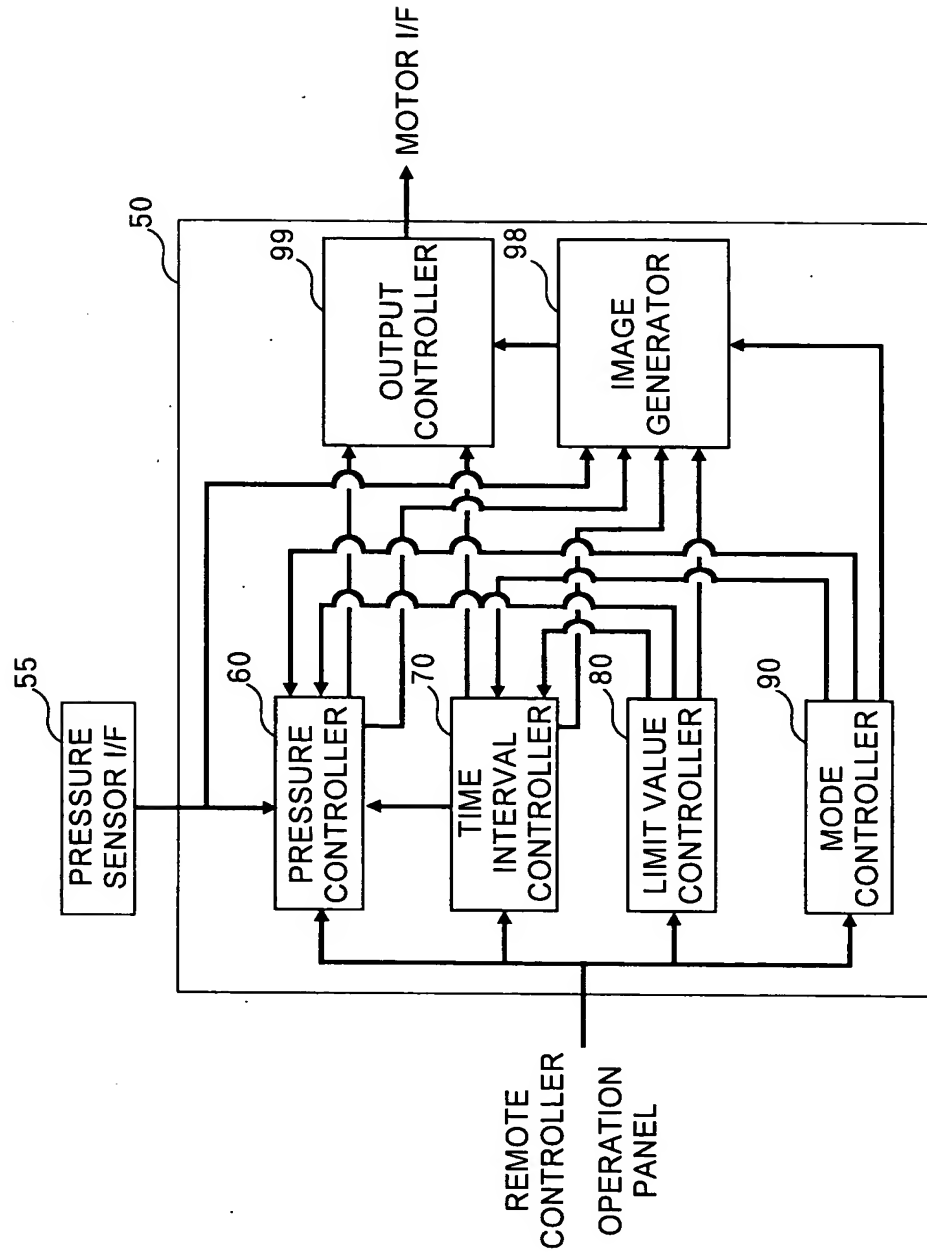


FIG. 6

6/21

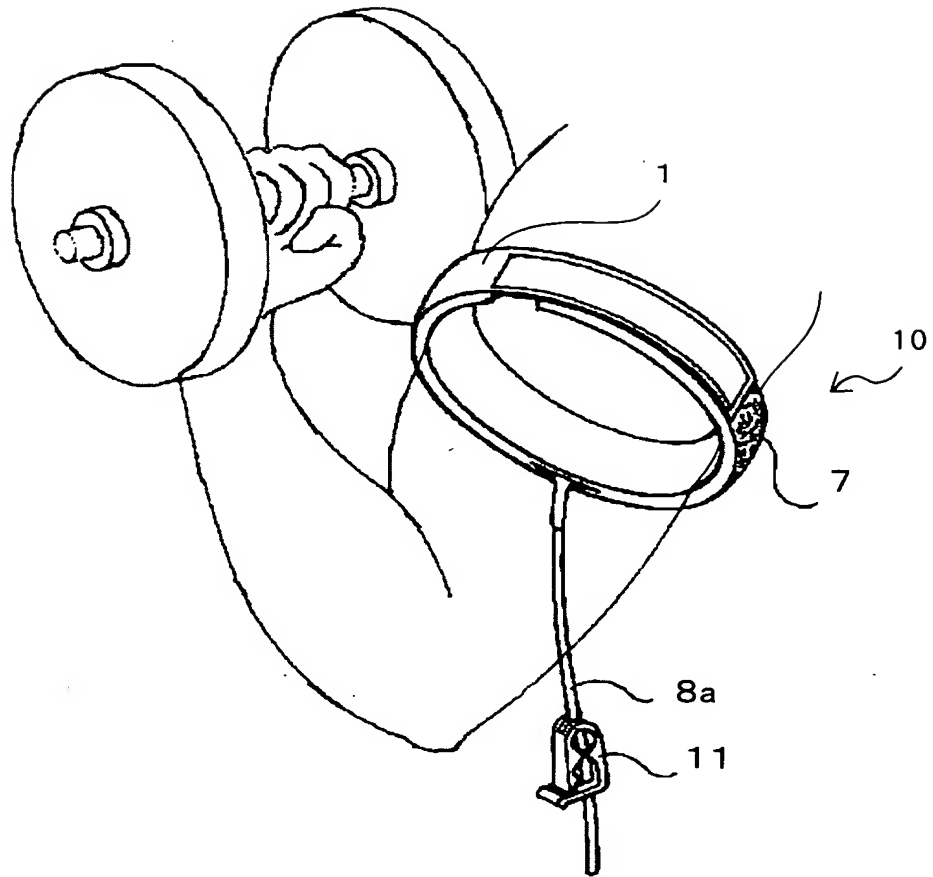


FIG. 7

7/21

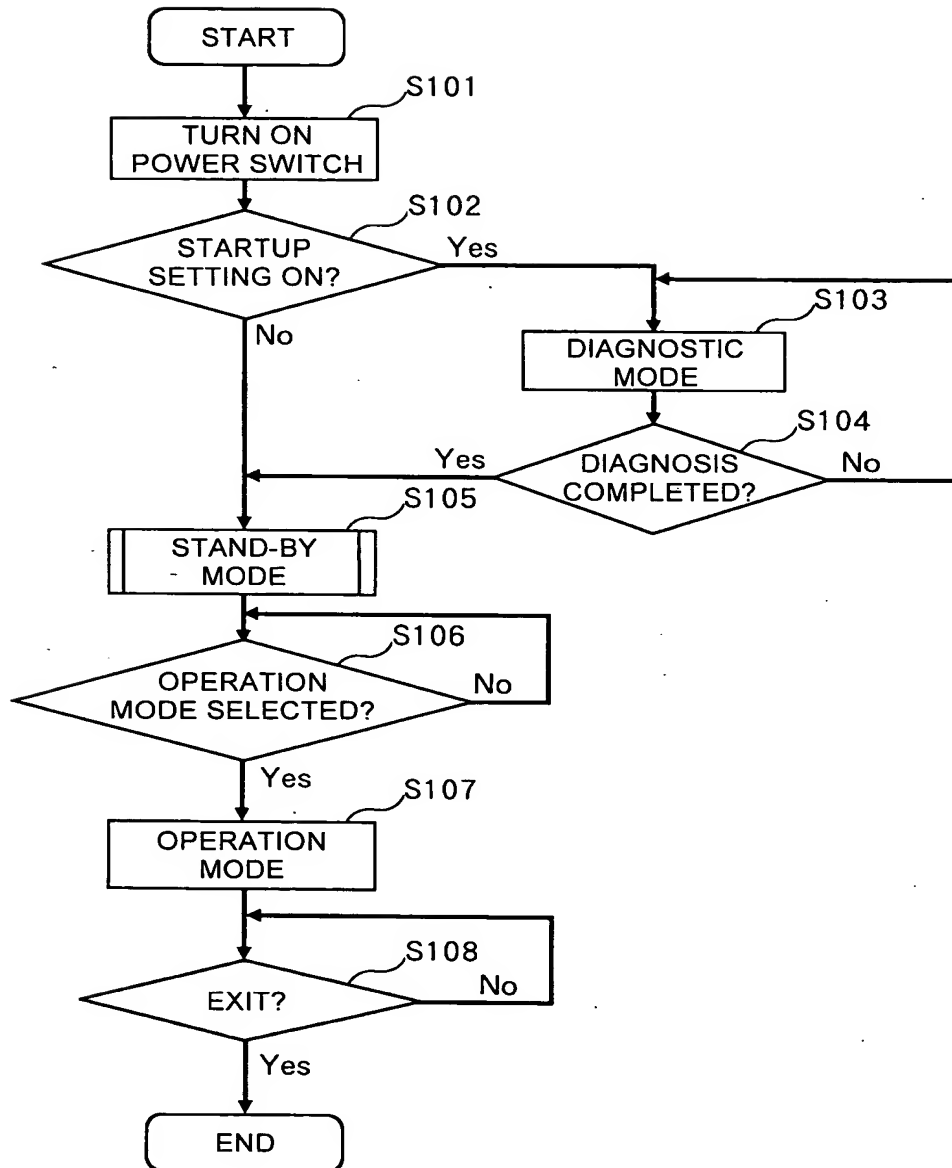


FIG. 8

8/21


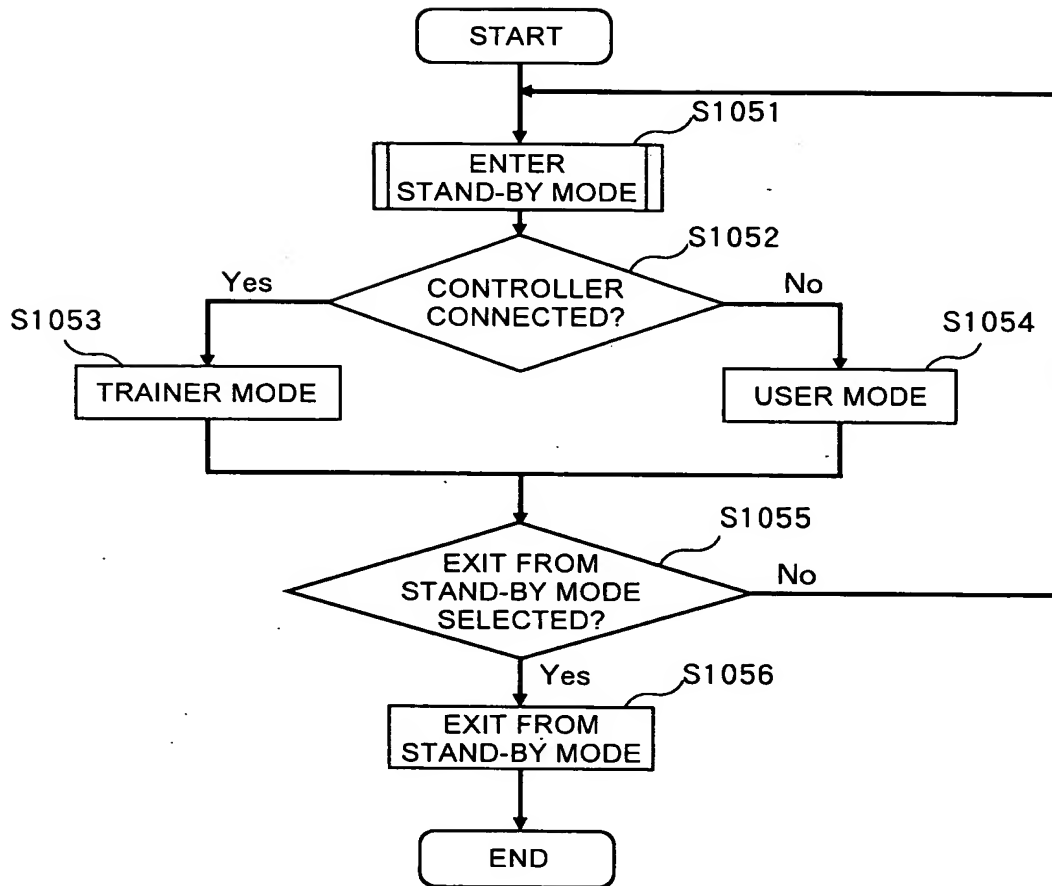


FIG. 9

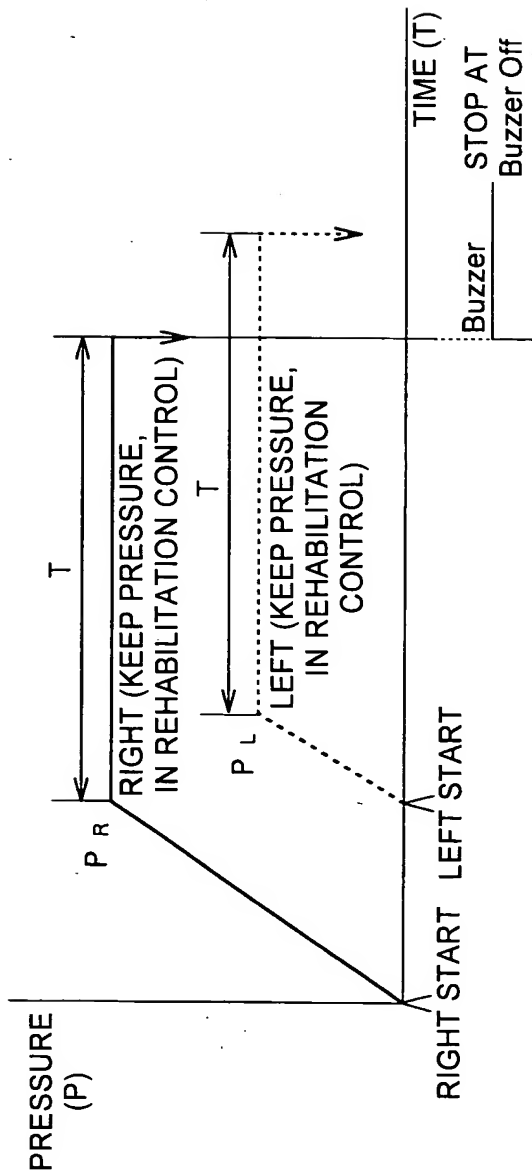

SETTING PARAMETERS				FACTORY DEFAULT SETTING
TIMER COUNT SETTING T		2-DIGIT NUMERIC VALUE	1 MINUIT UNIT	1
PRESSURE SETTING (USER)	RIGHT P _R	3-DIGIT NUMERIC VALUE	10 mmHg UNIT	100
	LEFT P _L	3-DIGIT NUMERIC VALUE	DITTO	100
PRESSURE SETTING (TRAINER)	RIGHT P _R	3-DIGIT NUMERIC VALUE	10 mmHg UNIT (UPPER LIMIT SETTING)	300
	LEFT P _L	3-DIGIT NUMERIC VALUE	DITTO	300

FIG. 10B

10/21

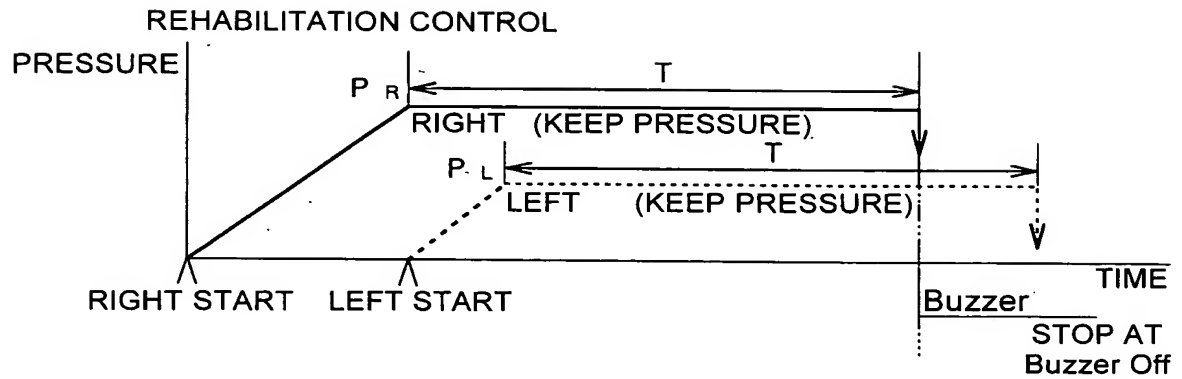


FIG. 11A

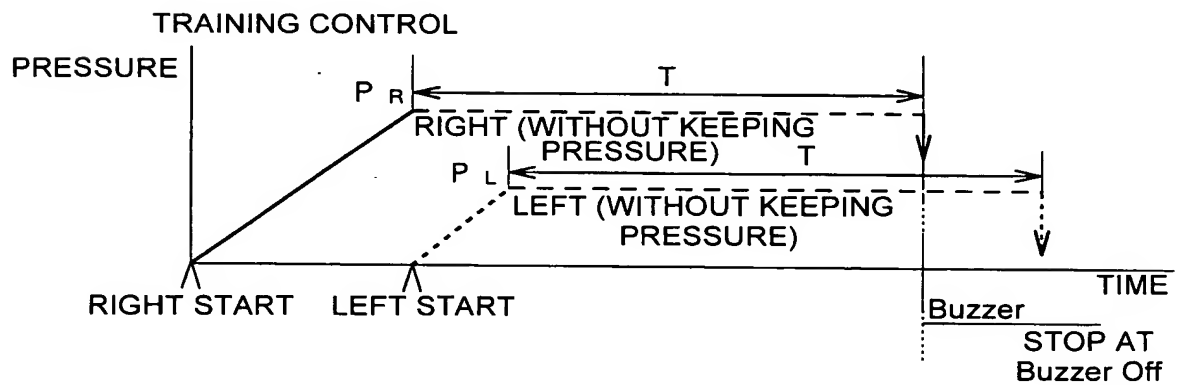


FIG. 11B

11/21

FIG. 12A

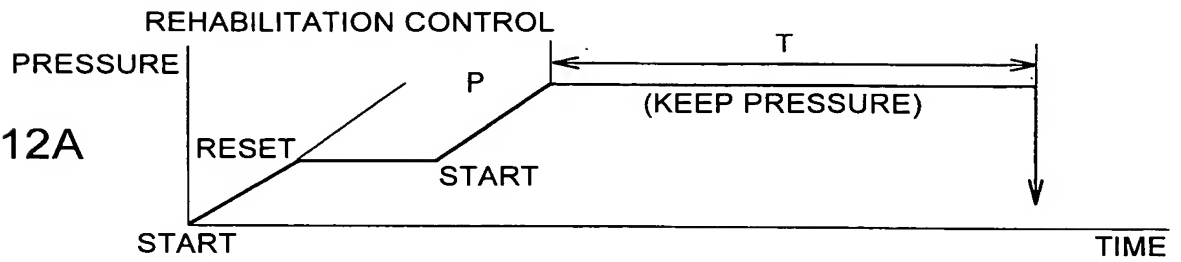


FIG. 12B

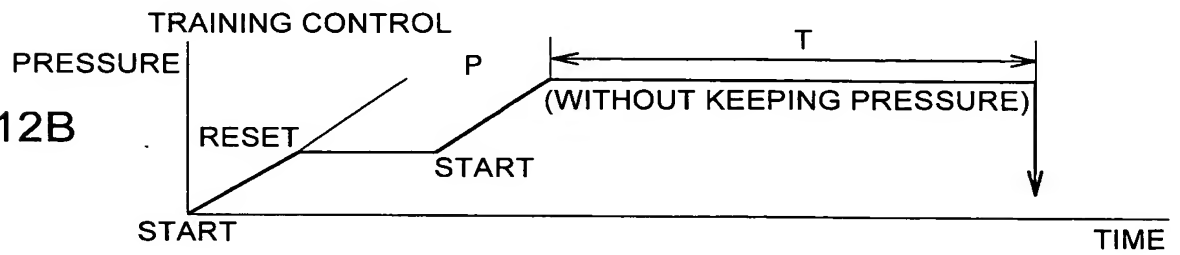


FIG. 12C

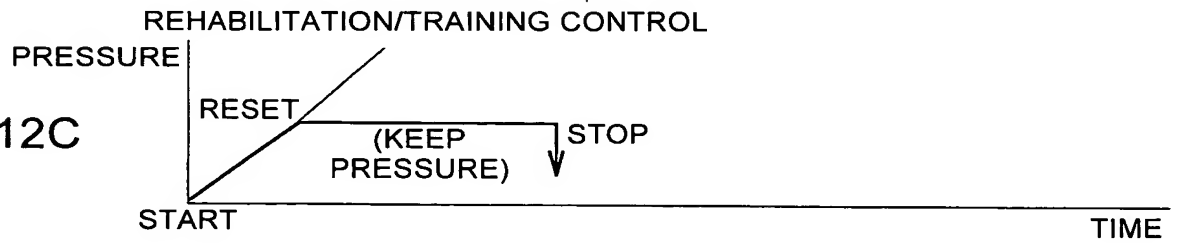


FIG. 12D

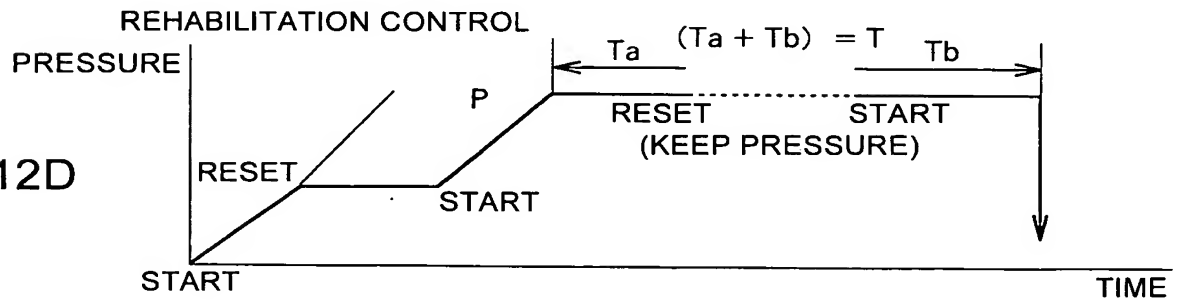
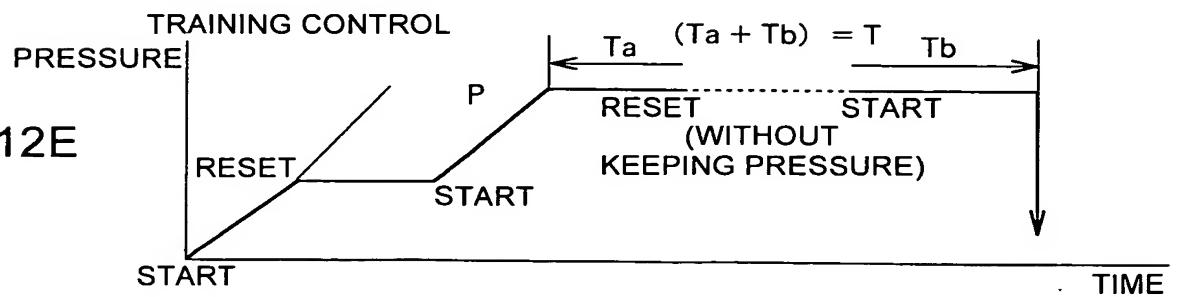


FIG. 12E



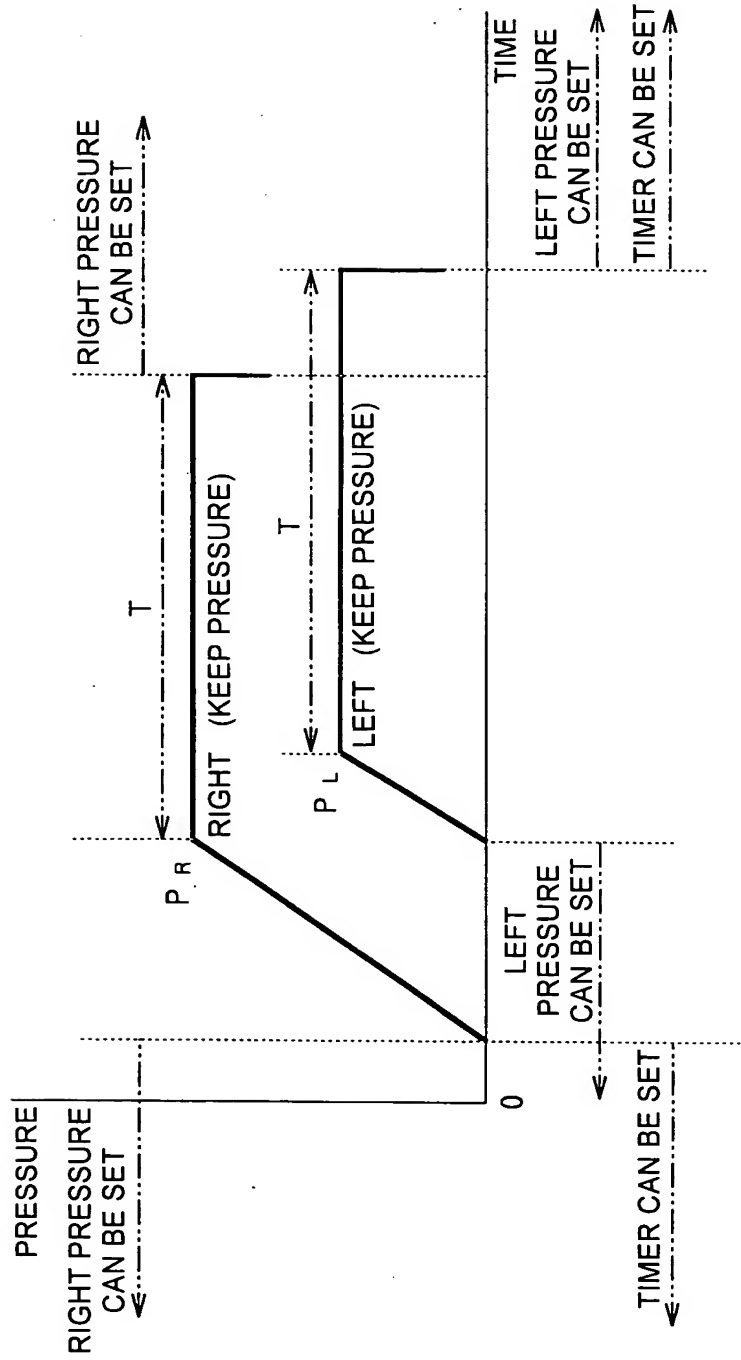


FIG. 13

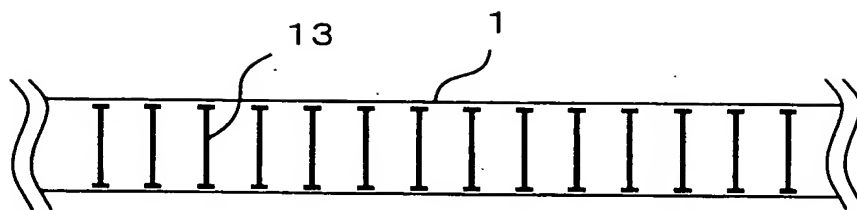


FIG. 14A

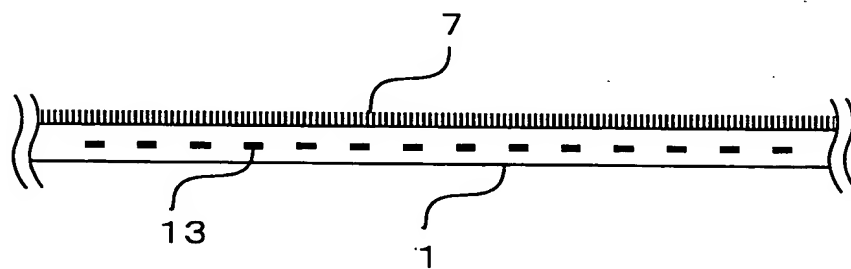


FIG. 14B

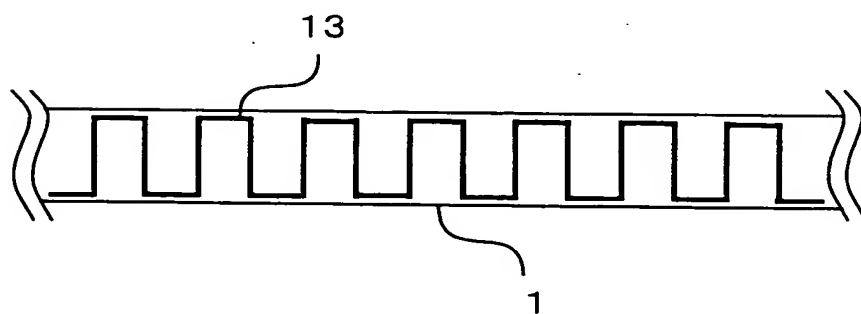


FIG. 15

14/21

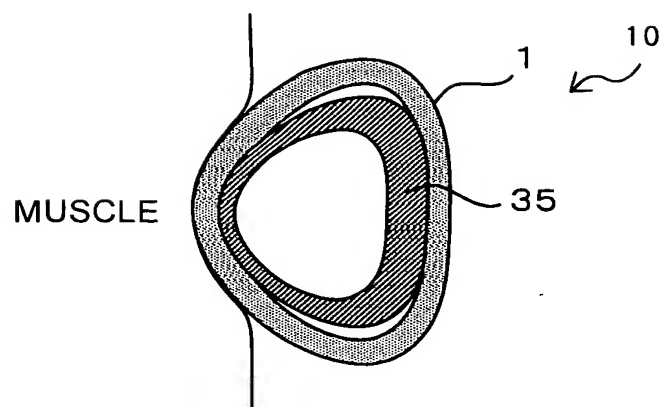


FIG. 16

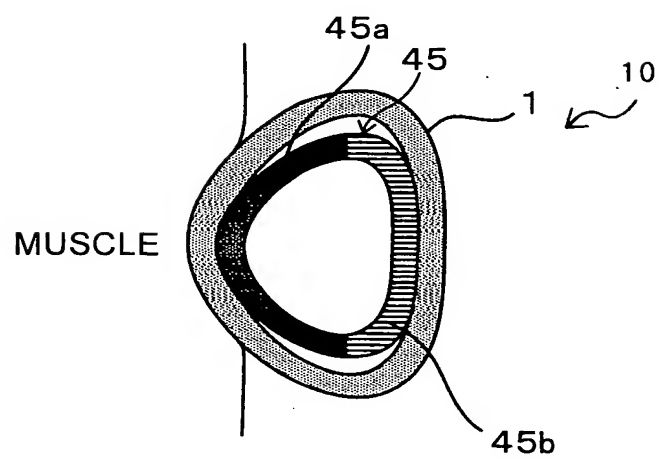


FIG. 17

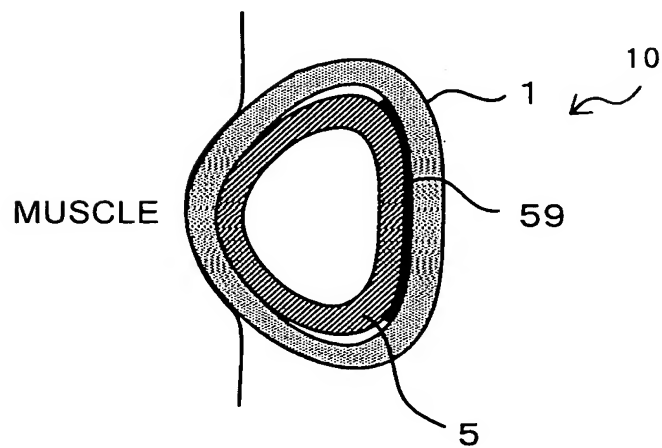


FIG. 18

15/21

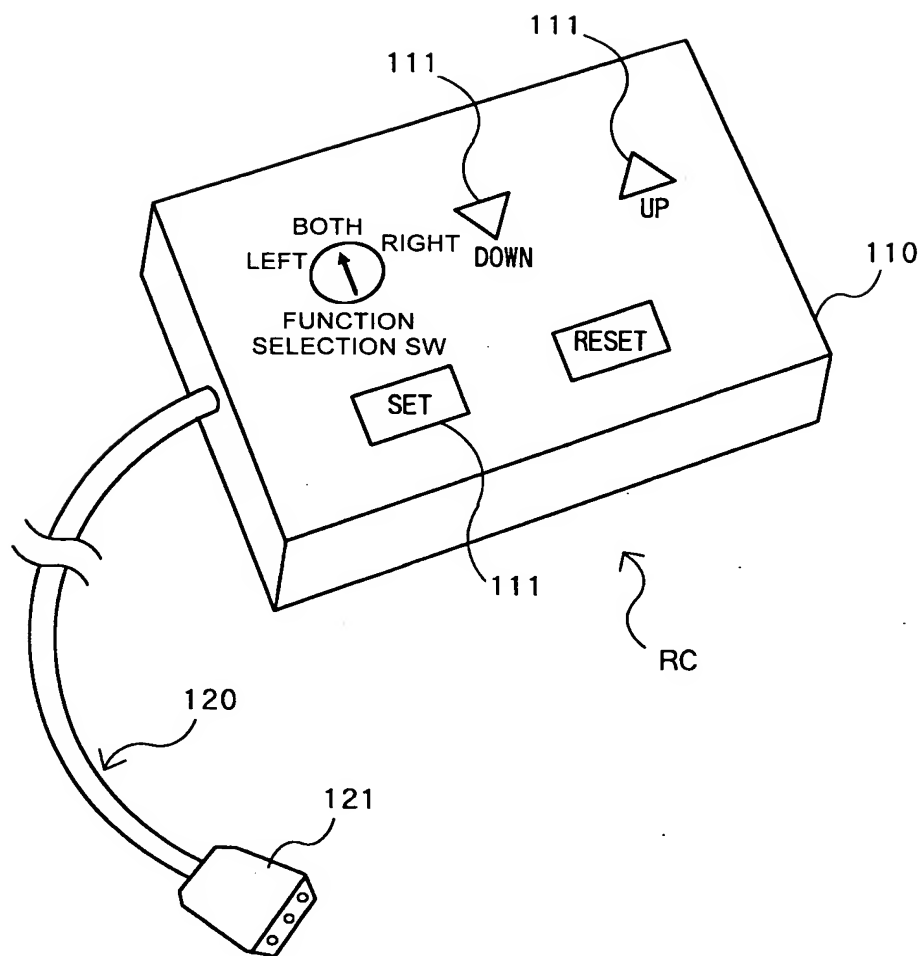


FIG. 19

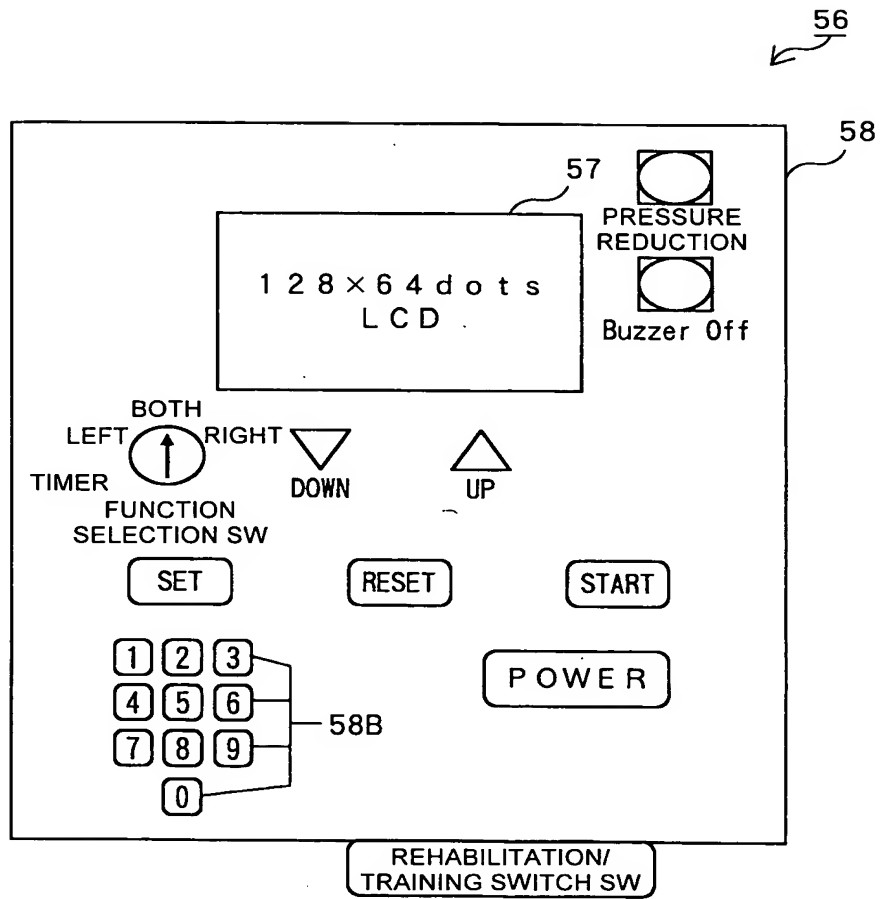


FIG. 20

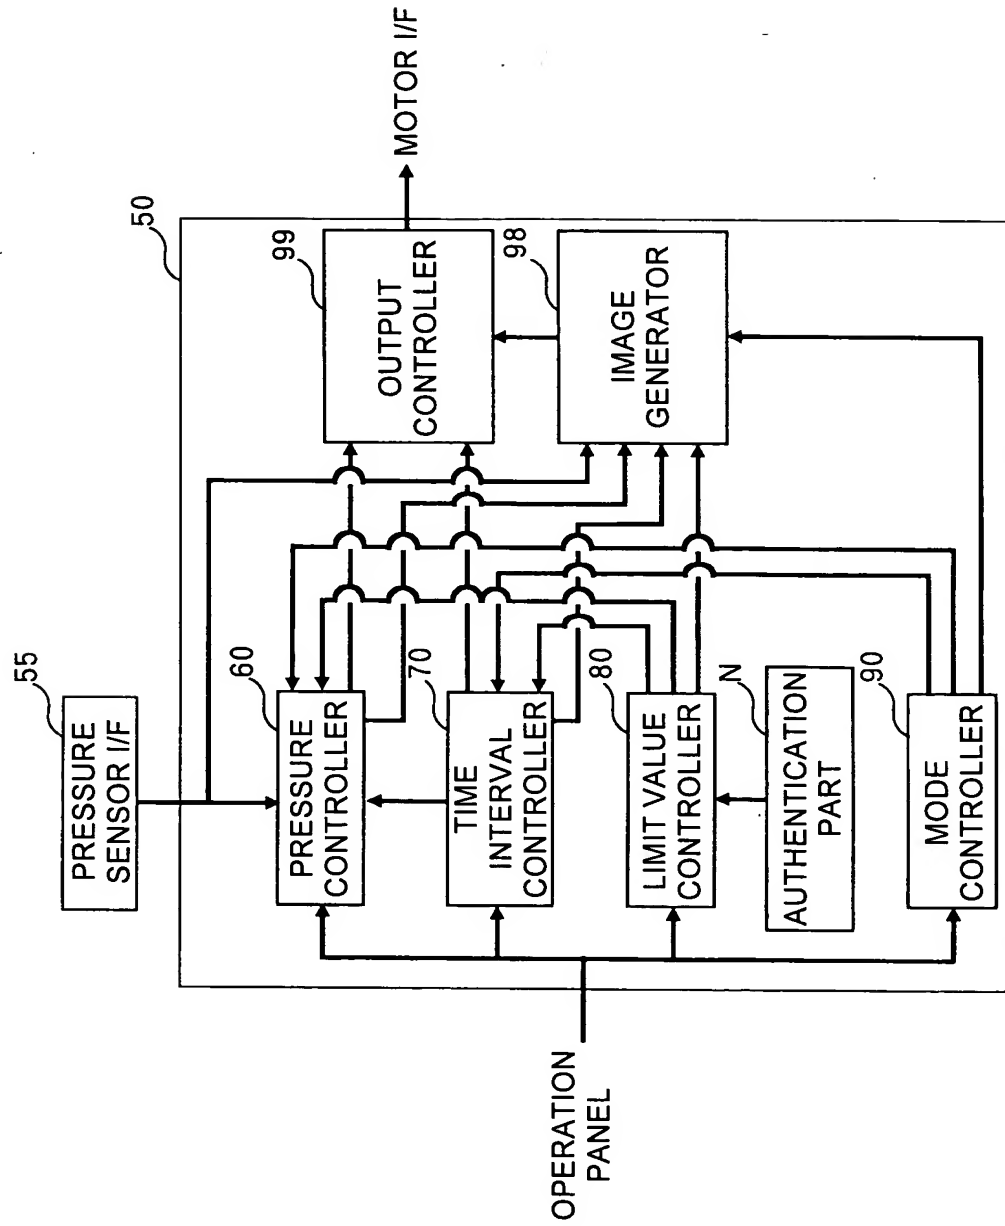


FIG. 21

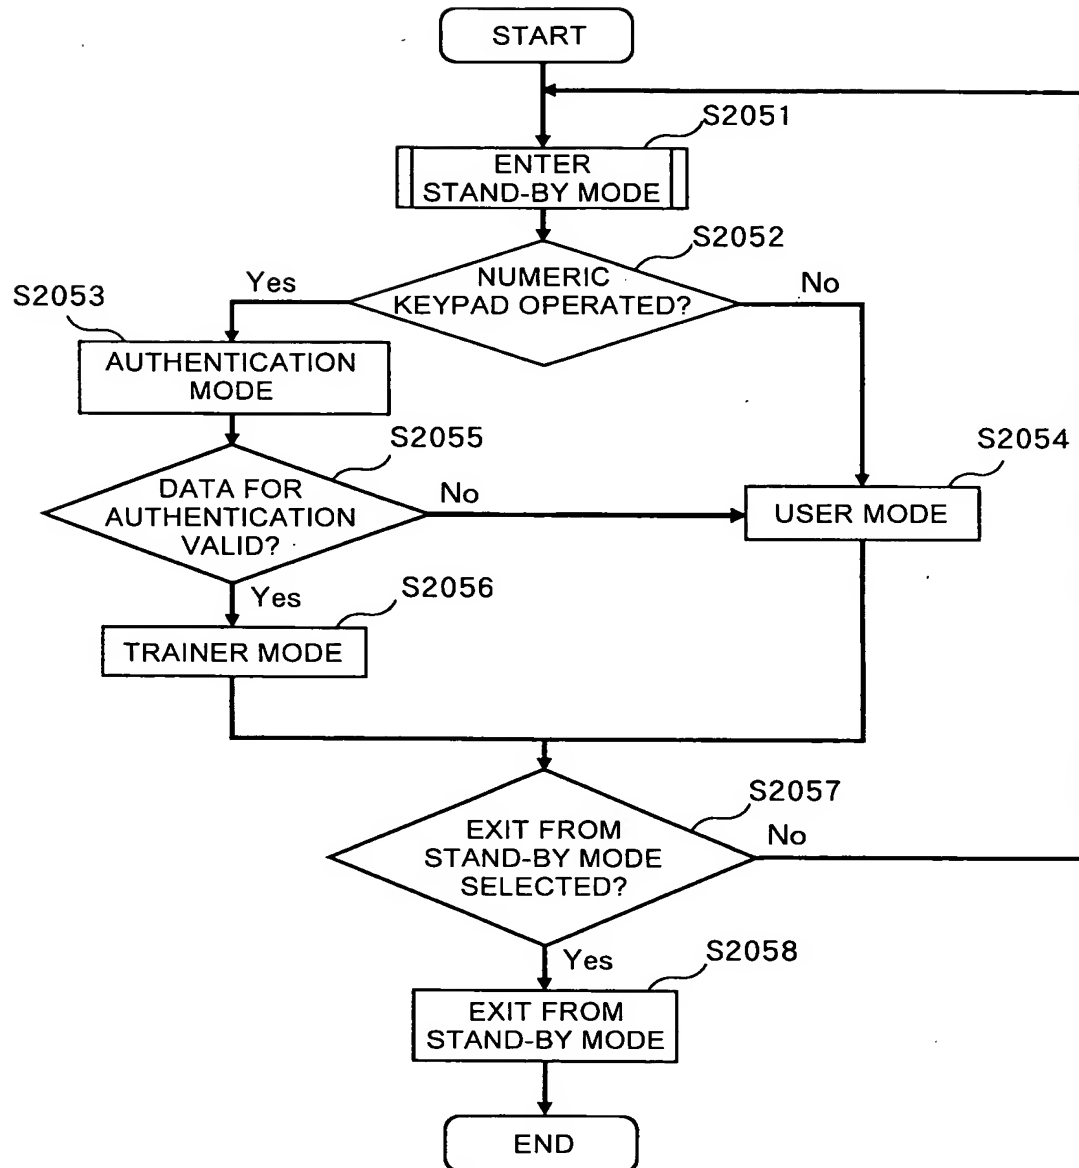


FIG. 22

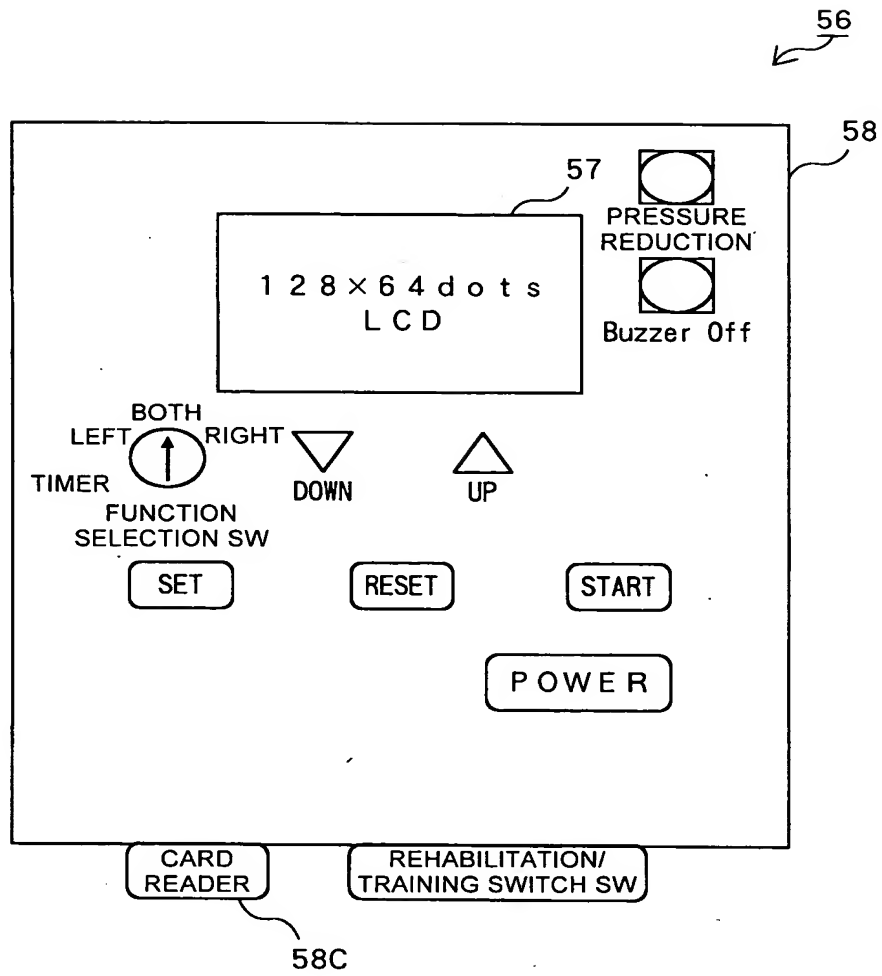


FIG. 23

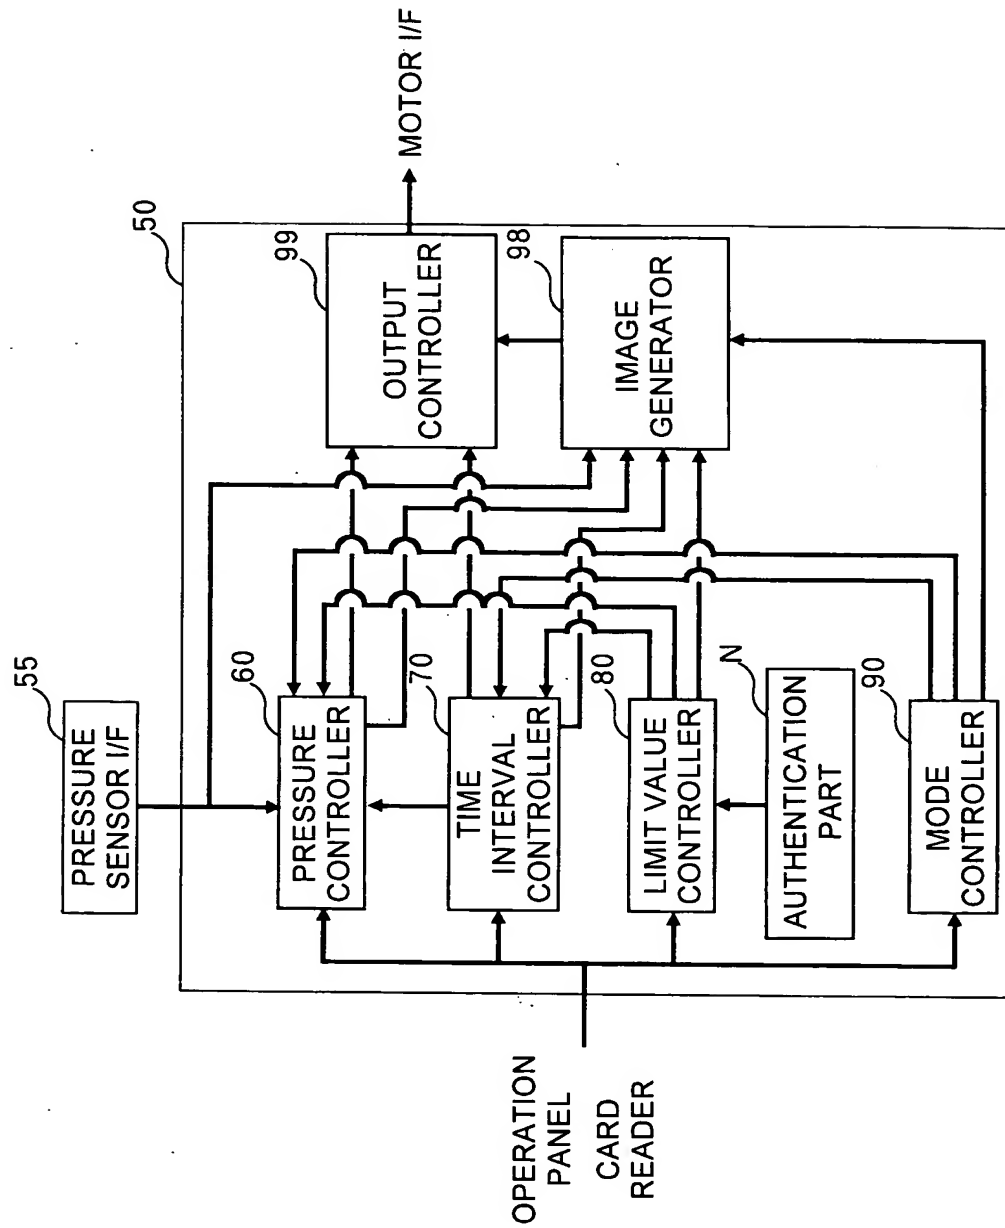


FIG. 24

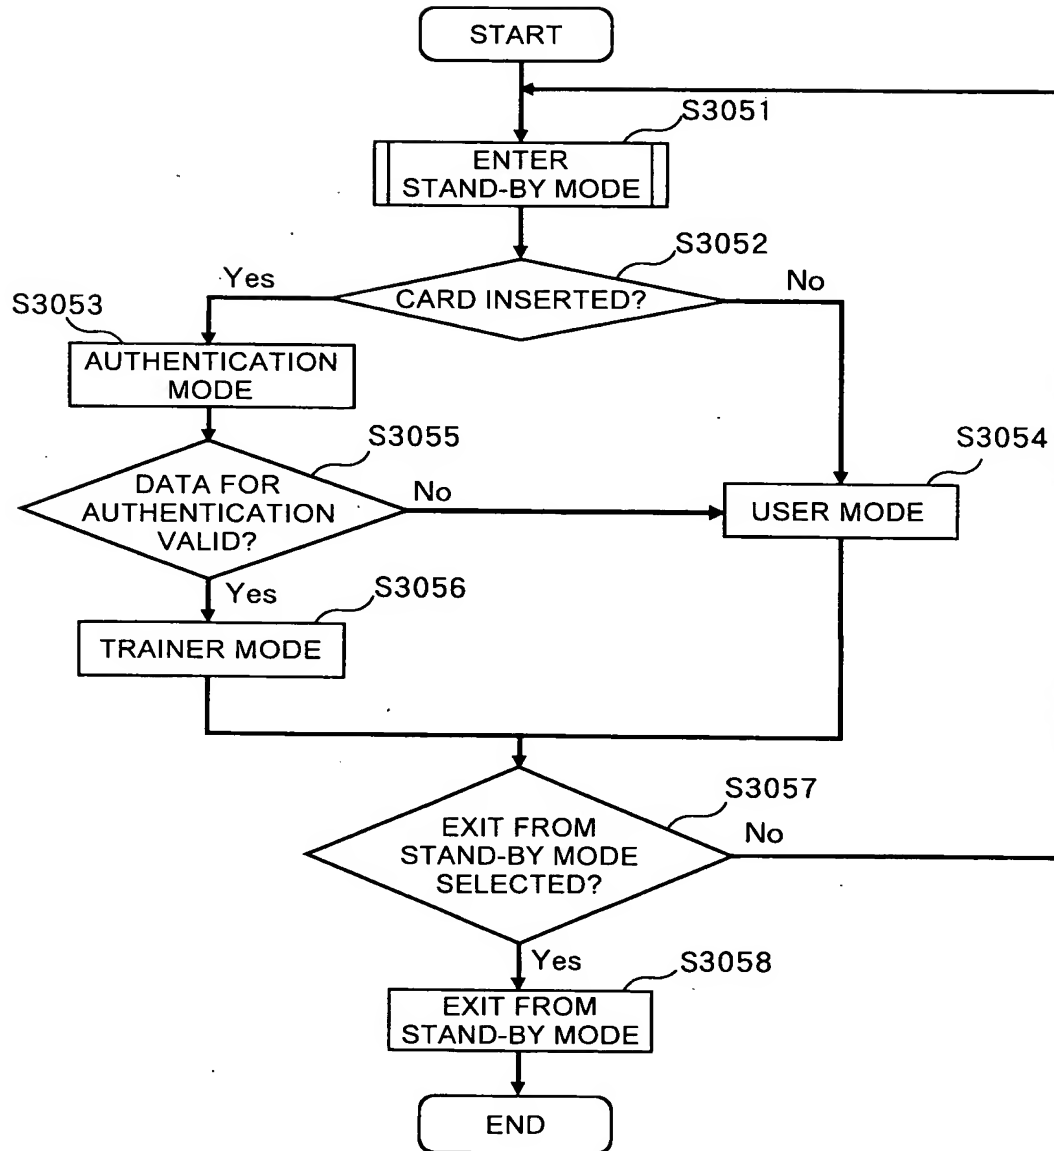


FIG. 25